

Telegesis™	 SILICON LABS	TG-UG-0502 ETRX3IPDDVK DevKit
ETRX357 IPD		User Guide 0502

Telegesis™ is a trademark of Silicon Laboratories Inc.

User Guide

Using Telegesis Demonstration Software with ETRX3 IPD and Mock Meter Firmware



IPD firmware version r300

Mock Meter firmware version r301

Smart Energy Demo Meter Version 0.1

Smart Energy In-Premise Display Version 0.1

Table of Contents

1	INTRODUCTION.....	2
2	INSTALLATION.....	2
2.1	Requirements.....	2
2.2	Instructions.....	2
2.2.1	ETRX3USB Driver.....	2
2.2.2	Mock Meter Demonstration Software	2
2.2.3	Smart Energy In-Premise Demonstration Software	3
2.2.4	Manual Installation of JAVA RxTx Library	3
3	USAGE	4
3.1	Mock Meter	4
3.1.1	Connection.....	4
3.1.2	Network Setup	6
3.1.3	Adding a Smart Energy Device to the Key Table.....	7
3.1.4	Permit Join.....	8
3.1.5	Basic Cluster.....	9
3.1.6	Time Cluster.....	10
3.1.7	Metering Cluster.....	11
3.1.8	Price Cluster	13
3.1.9	Messaging Cluster	14
3.2	In-Premise Display (IHD).....	15
3.2.1	Connection.....	15
3.2.2	Network Joining	17
3.2.3	Basic Cluster.....	18
3.2.4	IHD	19

1 Introduction

Telegesis have launched the SEP1.1 compliant ZigBee AT Command layer on the EM357 Ember platform. The ZigBee SEP AT commands allow developers to build a ZigBee Smart Energy compliant In-Premise Display without the need for any in-depth knowledge of the ZigBee PRO stack. To assist the user in practising with the IPD AT command set, a Mock Meter has been developed which can be used with the IPD for further development purposes.

Telegesis provides an example PC-based application to demonstrate the use of the In-premise Display firmware. The application allows the developer to understand the basic minimum required to create In-premise Display applications.

Note: the terms “In-Premise Display” and “In-Home Display” mean the same. We refer to the device as an In-Premise Display (IPD).

2 Installation

2.1 Requirements

The following is required for the demonstration to work:

- 1) Smart Energy Demo Kit containing
 - a. ETRX3USB-IPD
 - b. MockMeter (ETRX3USB)
- 2) ETRX3USB Windows Drivers
- 3) Mock Meter Demonstration Software Installer
- 4) Smart Energy Demonstration Software Installer

2.2 Instructions

2.2.1 ETRX3USB Driver

- 1) Download the ETRX3USB drivers from the Telegesis website using the following link:
www.silabs.com/telegesissoftware
- 2) Extract the file “TelegesisUSB Driver 6.6.1.zip” on the local hard drive
- 3) Run the file named “TGvcplInstaller.exe” and follow the onscreen prompts to complete the driver installation
- 4) Insert the ETRX3USB-IPD and the Mock Meter ETRX3USB for Windows to enumerate the devices

2.2.2 Mock Meter Demonstration Software

- 1) Download the Mock Meter application from the Telegesis website (www.silabs.com/telegesissoftware)
- 2) Run the file “SEMeterInstall.exe” and follow the onscreen prompts to complete the installation
- 3) The Mock Meter Installer will try to automatically point you install the JAVA Runtime Environment but if it fails then please install the latest version of Java on the computer manually by visiting the following link <http://java.com/en/download/>

2.2.3 Smart Energy In-Premise Demonstration Software

- 1) Download the Smart Energy In-Premise application from Telegesis website (www.silabs.com/telegesissoftware)
- 2) Run the file "SEIHDInstall.exe" and follow the onscreen prompts to complete the installation
- 3) The Smart Energy In-Premise Installer will try to automatically point you to install the JAVA Runtime Environment but if it fails then please install the latest version of Java on the computer manually by visiting the following link:
<http://java.com/en/download/>

2.2.4 Manual Installation of JAVA RxTx Library

Both the Mock Meter and the In-Premise Display applications connect to an ETRX3USB using a serial port and make use of the serial libraries made available under the project RxTx hosted at website <http://rxtx.qbang.org>. The Installer for the demo applications will install the library but it is known that the libraries are often removed when Java is updated hence making the demo application fail to detect or use any of the serial devices (ETRX3USBs).

Following the steps given below to install the Java RxTx library manually,

- 1) Download the latest pre-built binary from <http://rxtx.qbang.org>
- 2) Extract the "rxtxSerial.dll" to the "bin" directory of the Java install which is usually at "C:\Program Files\Java\jre7\bin" location
- 3) Extract the file "RxTxComm.jar" to the "lib\ext" directory of the Java install usually located at "C:\Program Files\Java\jre7\lib\ext"

3 Usage

3.1 Mock Meter


3.1.1 Connection

Insert the Mock Meter ETRX3USB into a USB slot on the PC.

If necessary, use the Windows Device Manager to find the COM port number of the Mock Meter.


Start the SEMeter application from the Windows Start Menu.

The following screen will be shown:

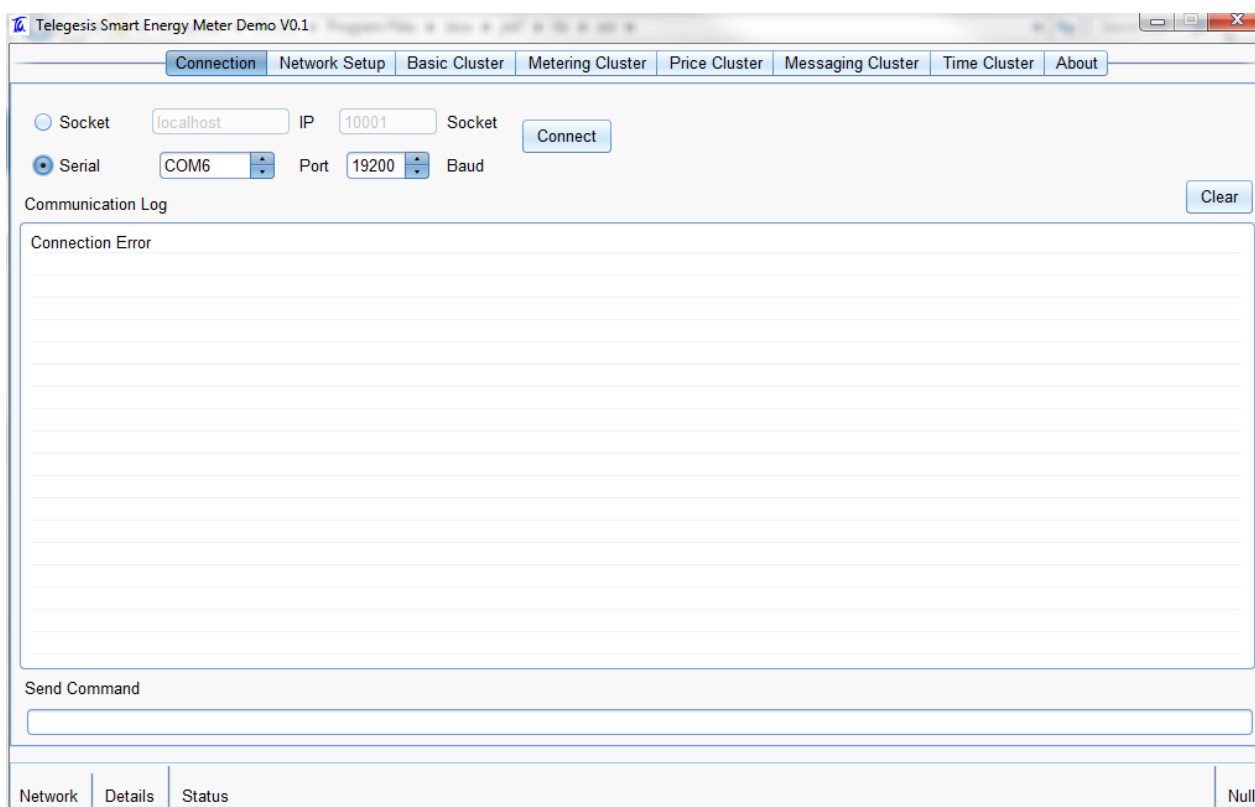

Click on the “Serial” radio button and select the serial port from the adjacent field. Click “Connect” to attempt to connect.

If the connection is successful the status bus is updated with Mock Meter information and ZigBee setup stored in the Mock Meter ETRX3USB is retrieved as shown in the screenshot below,

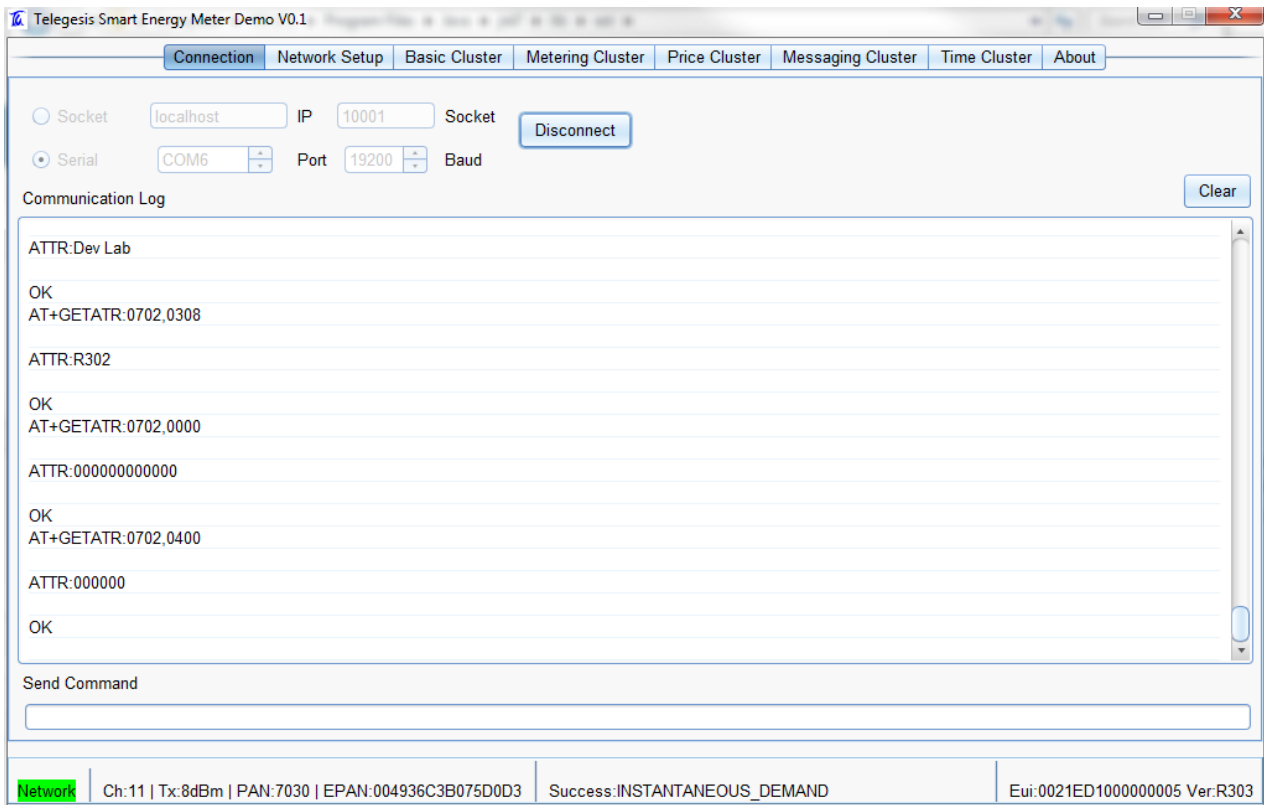

Telegesis Smart Energy Meter Demo V0.1

Connection Network Setup Basic Cluster Metering Cluster Price Cluster Messaging Cluster Time Cluster About

☐ Socket localhost IP 10001 Socket Disconnect
☒ Serial COM6 Port 19200 Baud

Communication Log Clear

```

ATTR:Dev Lab
OK
AT+GETATR:0702,0308

ATTR:R302
OK
AT+GETATR:0702,0000

ATTR:000000000000
OK
AT+GETATR:0702,0400

ATTR:000000
OK
  
```

Send Command


Network | Ch:11 | Tx:8dBm | PAN:7030 | EPAN:004936C3B075D0D3 | Success:INSTANTANEOUS_DEMAND | Eui:0021ED1000000005 Ver:R303

If the selected Serial Port does not connect to a Mock Meter ETRX3USB then an error is shown in the status bar.

All the messages exchanged between the Mock Meter ETRX3USB and the demonstration application are listed in the “Communication Log” window for reference and debugging. AT Commands can also be sent to the Mock Meter ETRX3USB by typing them into the “Send Command” field and pressing the “Enter” key.

3.1.2 Network Setup

Navigate to the “Network Setup” tab in the application; the following screen is presented:

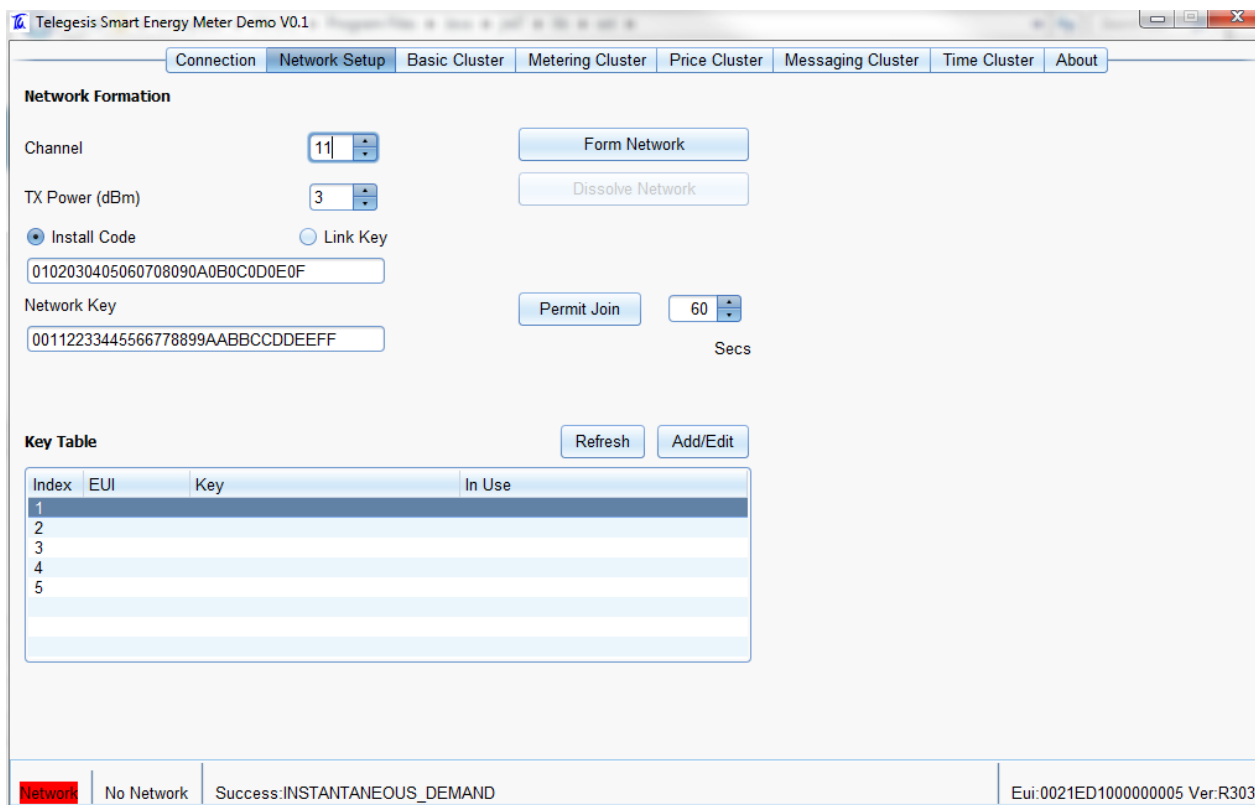

Telegesis Smart Energy Meter Demo V0.1

Connection **Network Setup** Basic Cluster Metering Cluster Price Cluster Messaging Cluster Time Cluster About

Network Formation

Channel: 11

TX Power (dBm): 3

☒ Install Code ☐ Link Key

0102030405060708090A0B0C0D0E0F

Network Key: 00112233445566778899AABBCCDDEEFF

Permit Join 60 Secs


Key Table Refresh Add/Edit

Index	EUI	Key	In Use
1			
2			
3			
4			
5			

Network No Network Success:INSTANTANEOUS_DEMAND Eui:0021ED1000000005 Ver:R303

To form a network,

- Select an appropriate ZigBee channel number and transmit power level for the device or use the default settings
- Using the radio button select whether the Trust Centre Link Key will be derived from an Install Code or whether the string given in the text below the radio button should be used as the Link Key.
- If Install Code is selected then give a string of 12,16,20 or 28 characters plus 4 character install code. Please note the two character make on hexadecimal number
- If “Link Key” is selected then enter a 32 character Link Key in ascii hexadecimal format.
- Enter a 32-character long Network key in the text box labelled “Network Key”
- Click the “Form Network” button to create the network with the above setting.
- If successful the following screen will be shown. Notice the status bar loaded with network information:

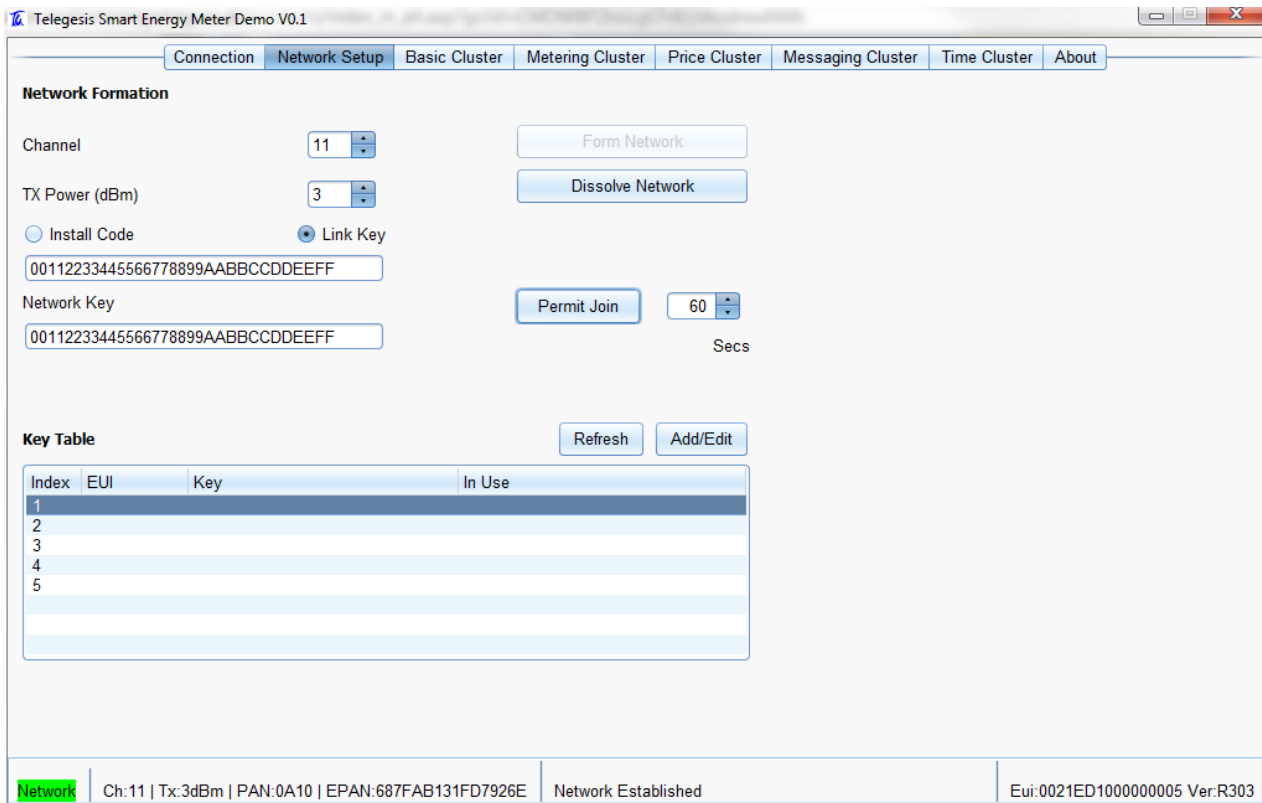

Telegesis Smart Energy Meter Demo V0.1

Connection | **Network Setup** | Basic Cluster | Metering Cluster | Price Cluster | Messaging Cluster | Time Cluster | About

Network Formation

Channel: 11

TX Power (dBm): 3

☐ Install Code ☒ Link Key

Network Key: 00112233445566778899AABBCCDDEEFF

Permit Join: 60 Secs

Key Table

Index	EUI	Key	In Use
1			
2			
3			
4			
5			


Refresh Add/Edit

Network | Ch: 11 | Tx: 3dBm | PAN: 0A10 | EPAN: 687FAB131FD7926E | Network Established | Eui: 0021ED1000000005 Ver: R303

3.1.3 Adding a Smart Energy Device to the Key Table

The security credentials of any device wishing to join the Smart Energy network must be entered in the Mock Meter which is the Trust Centre of the network.

In the picture shown above click on an empty row in the “Key Table” and click the “Add/Edit” button. The following screen is shown:

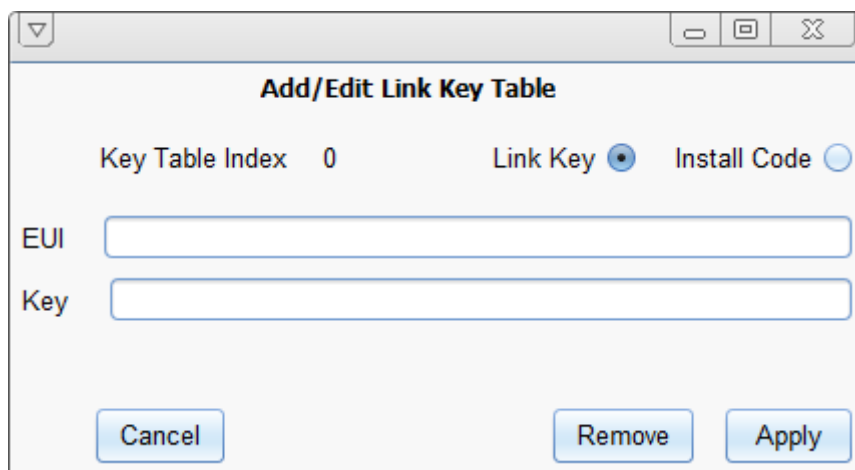

Add/Edit Link Key Table

Key Table Index: 0

☒ Link Key ☐ Install Code

EUI:

Key:

Cancel Remove Apply

Select the appropriate type as “Link Key” or the Install Code.

Fill in the EUI field with the hexadecimal IEEE64 address of the device wishing to join

Fill in the “Key” field with the “Link Key” or “Install Code” of the device wishing to join; the data entered must match with what is programmed in the joining device for the process to be successful.

Press “Apply” to write the entry into the “Key Table”.


Key Table				Refresh	Add/Edit
Index	EUI	Key	In Use		
1	0021ED1000000003	000102030405060708090A0B0C0D0E0F	False		
2					
3					
4					
5					

The field “In Use” changes to “True” once the device has joined and has successfully completed the CBKE process.

3.1.4 Permit Join

The ZigBee Smart Energy network will normally have the ZigBee joining turned off at the Trust Centre. When it is desired to allow a new device to join the network the network joining is allowed for a certain period of time only.

After adding the credentials of the joining device in the “Key Table” the network must be configured to allow joining to incoming devices. To do so select the number of seconds for which to allow joining and click “Permit Join”; the success of the operation will be indicated in the Status bar.

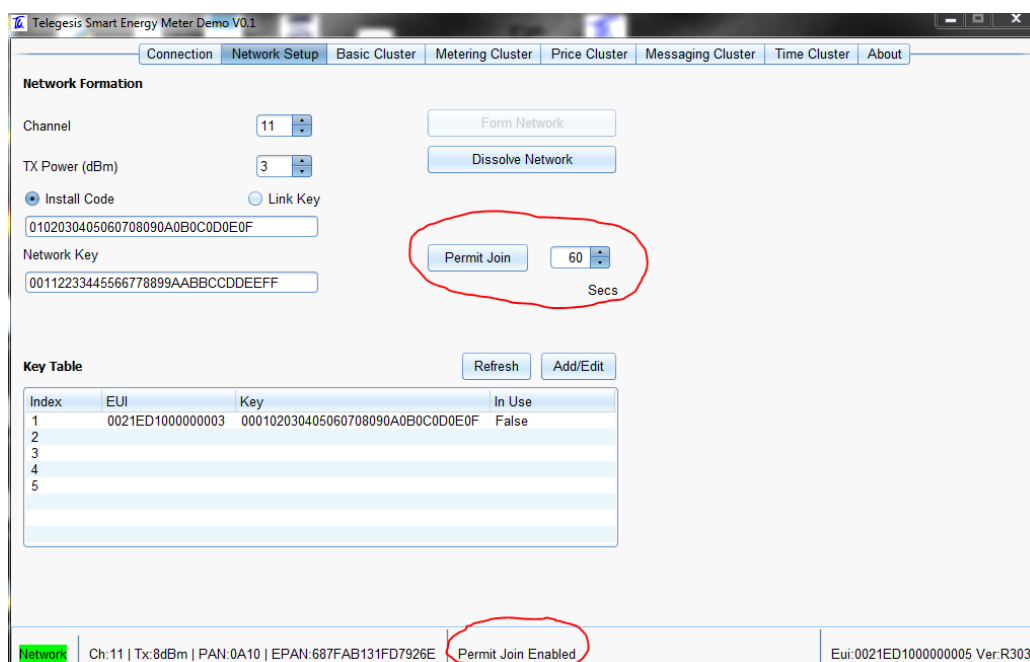

Telegesis Smart Energy Meter Demo V0.1

Connection | **Network Setup** | Basic Cluster | Metering Cluster | Price Cluster | Messaging Cluster | Time Cluster | About

Network Formation

Channel: 11

TX Power (dBm): 3

☒ Install Code ☐ Link Key

0102030405060708090A0B0C0D0E0F

Network Key: 00112233445566778899AABBCCDDEEFF

Permit Join 60 Secs

Key Table

Index	EUI	Key	In Use
1	0021ED1000000003	000102030405060708090A0B0C0D0E0F	False
2			
3			
4			
5			

Refresh Add/Edit


Network Ch: 11 | Tx: 8dBm | PAN: 0A10 | EPAN: 687FAB131FD7926E Permit Join Enabled Eui: 0021ED1000000005 Ver: R303

Once the Permit Join period has finished the status bar is updated accordingly

Network	Ch: 11 Tx: 8dBm PAN: 0A10 EPAN: 687FAB131FD7926E	Permit Join Finished	Eui: 0021ED1000000005 Ver: R303
---------	--	----------------------	---------------------------------

3.1.5 Basic Cluster

The Basic Cluster is mandatory for all devices in ZigBee Smart Energy Network. The attributes of the Basic Cluster hosted by the Mock Meter ETRX3USB can be seen by navigating to the “Basic Cluster” tab in the application. The following screen illustrates the Basic Cluster default settings in the Mock Meter ETRX3USB:

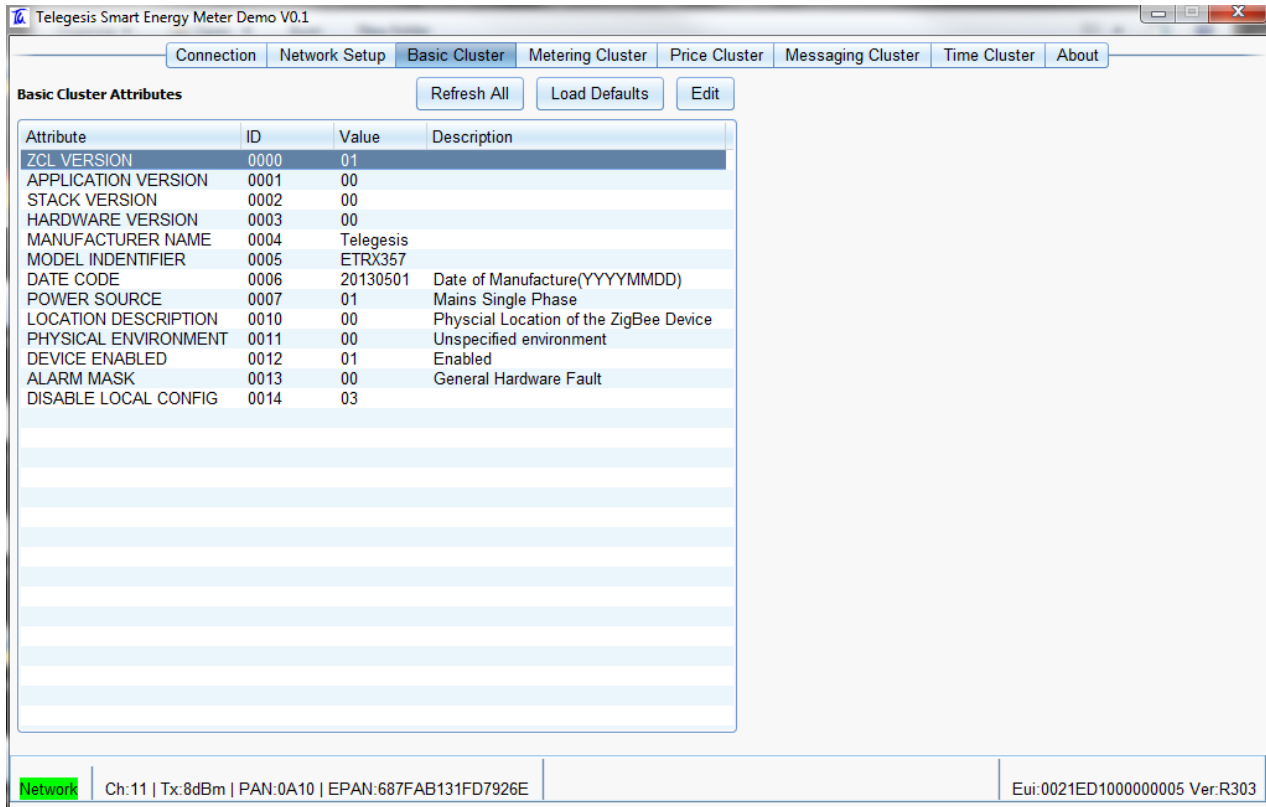

The screenshot shows the 'Basic Cluster Attributes' window of the 'Telegesis Smart Energy Meter Demo V0.1' application. The window has tabs for 'Connection', 'Network Setup', 'Basic Cluster' (selected), 'Metering Cluster', 'Price Cluster', 'Messaging Cluster', 'Time Cluster', and 'About'. Below the tabs are buttons for 'Refresh All', 'Load Defaults', and 'Edit'. The main area contains a table with the following data:

Attribute	ID	Value	Description
ZCL VERSION	0000	01	
APPLICATION VERSION	0001	00	
STACK VERSION	0002	00	
HARDWARE VERSION	0003	00	
MANUFACTURER NAME	0004	Telegesis	
MODEL IDENTIFIER	0005	ETRX357	
DATE CODE	0006	20130501	Date of Manufacture(YYYYMMDD)
POWER SOURCE	0007	01	Mains Single Phase
LOCATION DESCRIPTION	0010	00	Physical Location of the ZigBee Device
PHYSICAL ENVIRONMENT	0011	00	Unspecified environment
DEVICE ENABLED	0012	01	Enabled
ALARM MASK	0013	00	General Hardware Fault
DISABLE LOCAL CONFIG	0014	03	


At the bottom of the window, there is a status bar with the following information: Network | Ch:11 | Tx:8dBm | PAN:0A10 | EPAN:687FAB131FD7926E | Eui:0021ED1000000005 Ver:R303

All the attributes listed in the table above can be changed by double clicking on the attribute row or by clicking on the “Edit” button.

Please ensure that when updating the attributes the data must conform to the specifications to ensure proper application behaviour.

3.1.6 Time Cluster

The Mock Meter ETRX3USB need to be set up with the current time as well as being declared as the master time source of the network in the Time Status attribute. The “Time Cluster” tab gives access to the Time Cluster attributes of the Mock Meter.

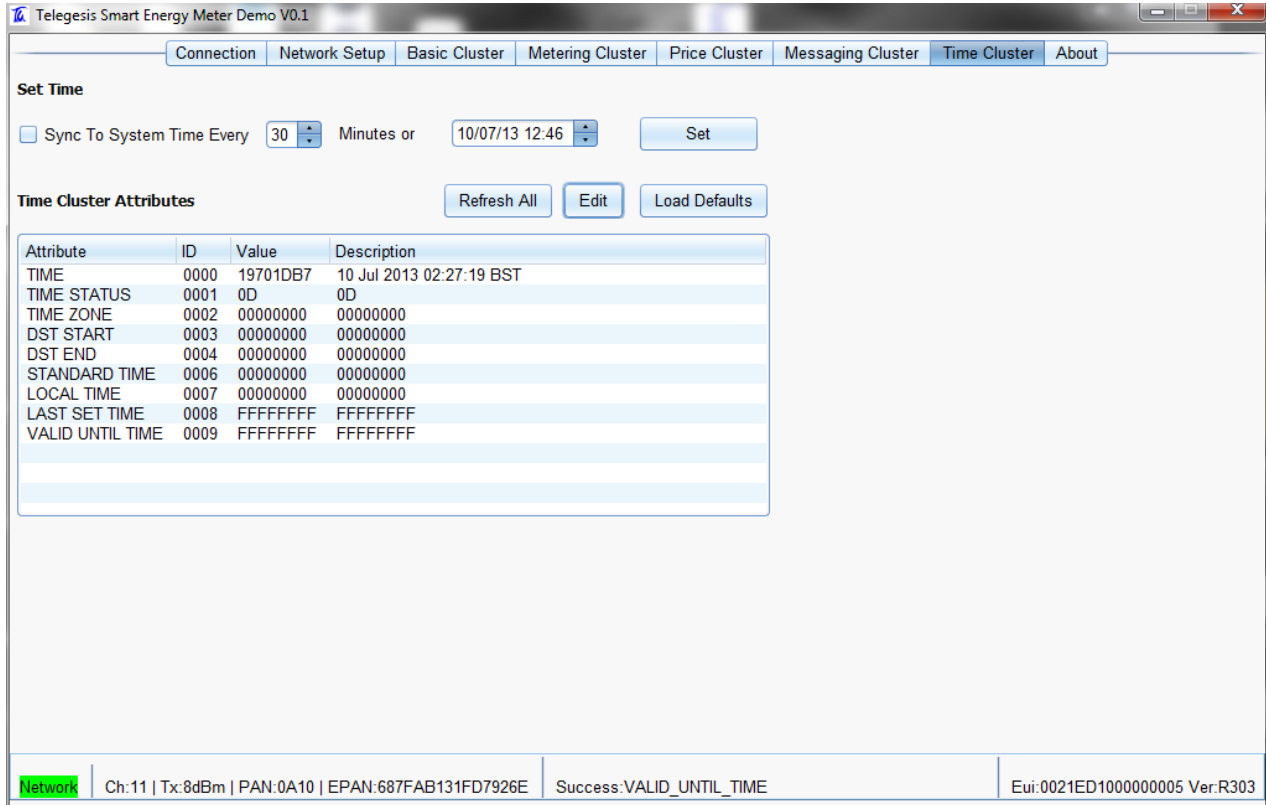

The screenshot shows the 'Time Cluster' tab of the 'Telegesis Smart Energy Meter Demo V0.1' application. The interface includes a 'Set Time' section with a checkbox for 'Sync To System Time Every 30 Minutes or 10/07/13 12:46' and a 'Set' button. Below this is the 'Time Cluster Attributes' section with 'Refresh All', 'Edit', and 'Load Defaults' buttons. A table lists various time-related attributes with their IDs, values, and descriptions.

Attribute	ID	Value	Description
TIME	0000	19701DB7	10 Jul 2013 02:27:19 BST
TIME STATUS	0001	0D	0D
TIME ZONE	0002	00000000	00000000
DST START	0003	00000000	00000000
DST END	0004	00000000	00000000
STANDARD TIME	0006	00000000	00000000
LOCAL TIME	0007	00000000	00000000
LAST SET TIME	0008	FFFFFFFF	FFFFFFFF
VALID UNTIL TIME	0009	FFFFFFFF	FFFFFFFF


At the bottom of the window, a status bar displays network information: Network | Ch:11 | Tx:8dBm | PAN:0A10 | EPAN:687FAB131FD7926E | Success:VALID_UNTIL_TIME | Eui:0021ED1000000005 Ver:R303

Check the checkbox “Sync Time to System Time” to enable syncing the time of the Mock Meter with the computer. The time in the Mock Meter may drift over time so the application allows for syncing the time with the PC periodically.

The Mock Meter can be made the Master Time source of the network by editing the “TIME STATUS” attribute or by loading the defaults using the “Load Defaults” button.

3.1.7 Metering Cluster

The “Metering Cluster” tab gives access to the attributes hosted by the metering cluster as shown below:

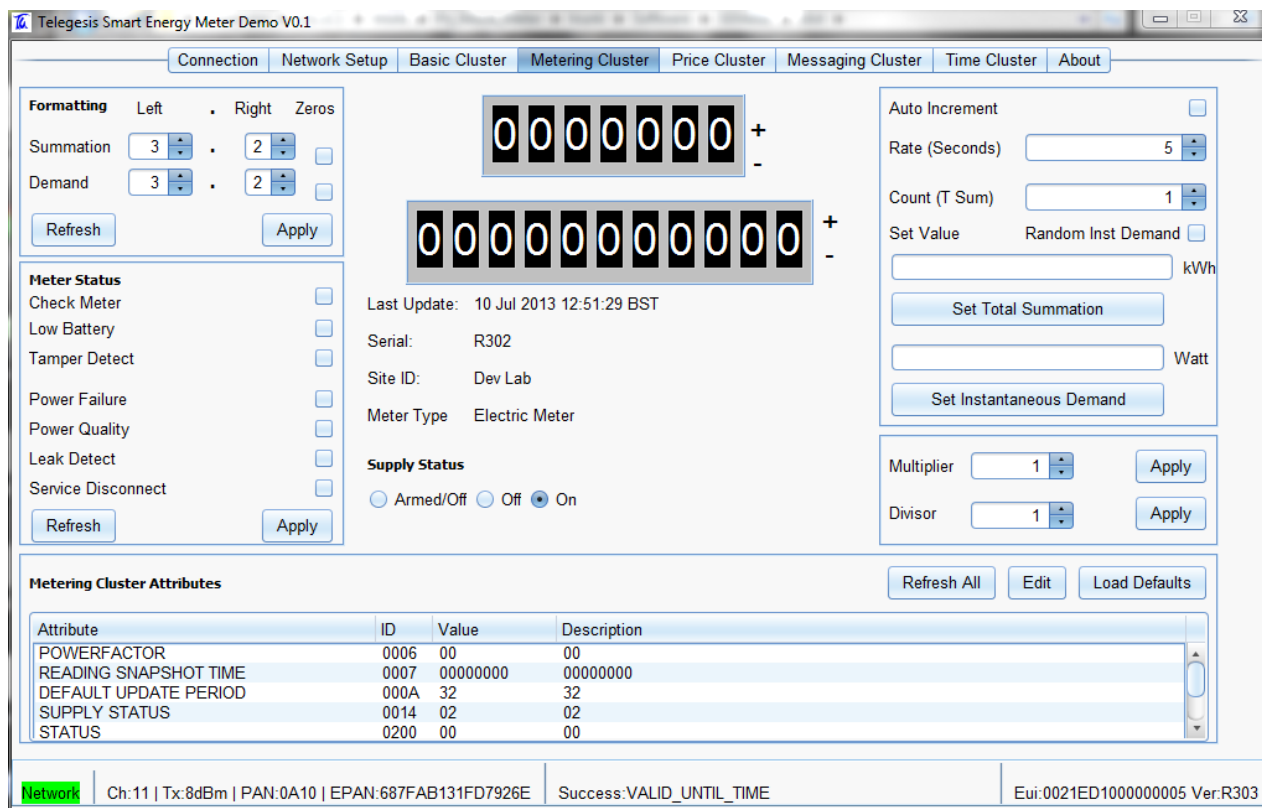


The screenshot shows the 'Metering Cluster' tab of the Telegesis Smart Energy Meter Demo V0.1 application. The interface includes several sections:

- Formatting:** Controls for 'Left', 'Right', and 'Zeros' for 'Summation' and 'Demand' attributes. 'Summation' is set to 3 left and 2 right zeros. 'Demand' is set to 3 left and 2 right zeros. There are 'Refresh' and 'Apply' buttons.
- Meter Status:** A list of status indicators with checkboxes: Check Meter, Low Battery, Tamper Detect, Power Failure, Power Quality, Leak Detect, and Service Disconnect. There are 'Refresh' and 'Apply' buttons.
- Central Display:** Two large digital displays showing '00000000' and '000000000000'. Below them, it shows 'Last Update: 10 Jul 2013 12:51:29 BST', 'Serial: R302', 'Site ID: Dev Lab', and 'Meter Type: Electric Meter'.
- Supply Status:** Radio buttons for 'Armed/Off', 'Off', and 'On' (selected).
- Auto Increment Section:** Includes an 'Auto Increment' checkbox, 'Rate (Seconds)' set to 5, 'Count (T Sum)' set to 1, and a 'Random Inst Demand' checkbox. There are buttons for 'Set Total Summation' and 'Set Instantaneous Demand'.
- Multiplier and Divisor:** 'Multiplier' is set to 1 and 'Divisor' is set to 1, both with 'Apply' buttons.
- Metering Cluster Attributes Table:**

Attribute	ID	Value	Description
POWERFACTOR	0006	00	00
READING SNAPSHOT TIME	0007	00000000	00000000
DEFAULT UPDATE PERIOD	000A	32	32
SUPPLY STATUS	0014	02	02
STATUS	0200	00	00
- Footer:** Network status (Ch: 11 | Tx: 8dBm | PAN: 0A10 | EPAN: 687FAB131FD7926E), Success: VALID_UNTIL_TIME, and Eui: 0021ED1000000005 Ver: R303.

To set the meter to auto-increment its current summation attribute the “Auto Increment” check box can be checked which will make the application update the Current Summation attribute as specified in the field “Count (T Sum)” and at the rate specified by “Rate (Seconds)” field. If the “Random Inst Demand” button is checked a random value between 0 and 1000 watts will be set in the Instantaneous Demand attribute at each interval as specified by the “Rate (Seconds)” field.

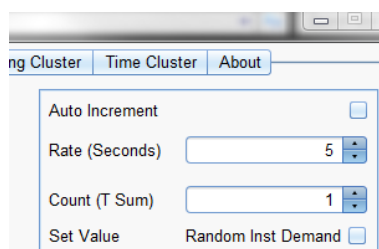


This close-up shows the 'Auto Increment' section of the interface. It includes the 'Auto Increment' checkbox, the 'Rate (Seconds)' field set to 5, the 'Count (T Sum)' field set to 1, and the 'Random Inst Demand' checkbox.

The values for Total Summation and Instantaneous Demand can also be updated via the “Set Total Summation” and “Set Instantaneous Demand” buttons.

The values shown on the meter dial for Total Summation such as given below are calculated as:

$$\text{Dial Value} = \text{Total Summation Attribute Value} * \text{Multiplier} / \text{Divisor}$$

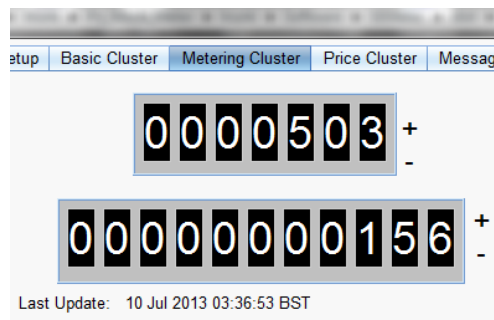


Setup | Basic Cluster | **Metering Cluster** | Price Cluster | Message

0000503 +
-

00000000156 +
-

Last Update: 10 Jul 2013 03:36:53 BST

Meter Status can be updated by clicking on the required check boxes and clicking the “Apply” button in the following section of the “Metering Cluster” tab:

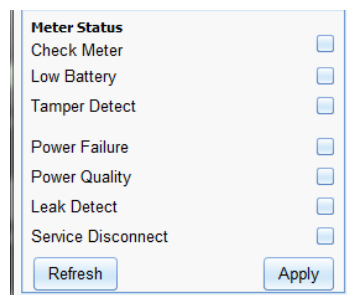

Meter Status

Check Meter ☐

Low Battery ☐

Tamper Detect ☐

Power Failure ☐

Power Quality ☐

Leak Detect ☐

Service Disconnect ☐


Refresh Apply

Most of the attributes can be updated by editing the rows in the “Metering Cluster Attributes” table by either double clicking the relevant row or clicking on the “Edit” button.

Metering Cluster Attributes				Refresh All	Edit	Load Defaults
Attribute	ID	Value	Description			
POWERFACTOR	0006	00	00			
READING SNAPSHOT TIME	0007	19702E05	19702E05			
DEFAULT UPDATE PERIOD	000A	32	32			
SUPPLY STATUS	0014	02	02			
STATUS	0200	00	00			

3.1.8 Price Cluster

The price set in the “Price Cluster” can then be published to or retrieved by an IHD. The Mock Meter ETRX3USB can store up to 5 prices, one of the 5 stored (usually at index 1) is the current price and the remainder should be scheduled prices and should not overlap each other in time.

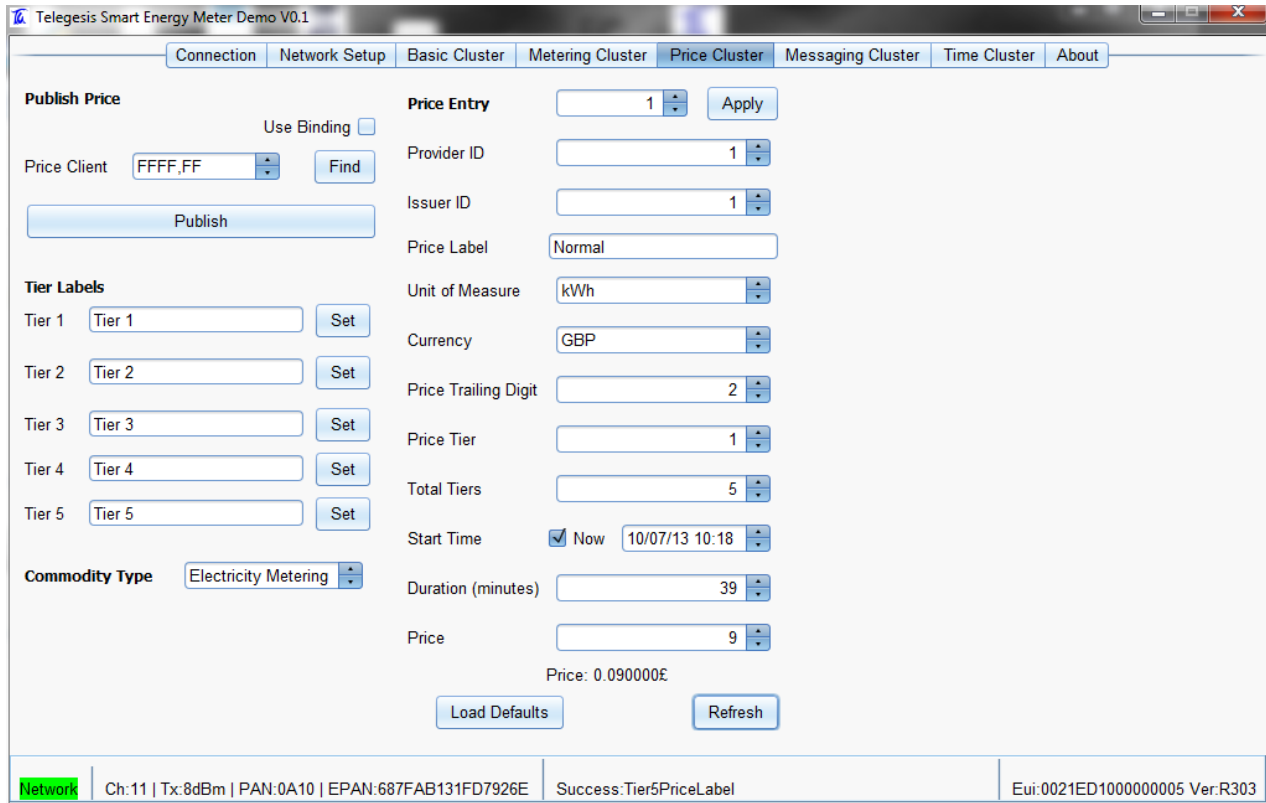

Telegesis Smart Energy Meter Demo V0.1

Connection | Network Setup | Basic Cluster | Metering Cluster | **Price Cluster** | Messaging Cluster | Time Cluster | About

Publish Price

Use Binding ☐

Price Client: FFFF,FF

Tier Labels

Tier 1: Tier 1

Tier 2: Tier 2

Tier 3: Tier 3

Tier 4: Tier 4

Tier 5: Tier 5

Commodity Type: Electricity Metering

Price Entry

Price Entry: 1

Provider ID: 1

Issuer ID: 1

Price Label: Normal

Unit of Measure: kWh

Currency: GBP

Price Trailing Digit: 2

Price Tier: 1

Total Tiers: 5

Start Time: ☒ Now 10/07/13 10:18

Duration (minutes): 39

Price: 9

Price: 0.090000£

Network | Ch:11 | Tx:8dBm | PAN:0A10 | EPAN:687FAB131FD7926E | Success:Tier5PriceLabel | Eui:0021ED1000000005 Ver:R303


Change the “Price Entry” spinner to see the prices contained in the respective entries in the price table of the Mock Meter ETRX3USB.

Make the necessary changes to the price table entry and then click “Apply” to make that entry active. Only entries made active can be sent to or retrieved by the IHD. See ZSE1.1 specification for description of various fields of the price table entry.

The price can be published to a client by use of ZigBee binding provided that the Price Client has set the binding in the Mock Meter ETRX3USB during ZSE registration process or by discovering the Price Client and then publishing the price to it. Select the appropriate option in the “Price Cluster” tab for either publishing to a “Price Client” using the address discovered using the “Find” button or by using the “Use Binding” check box and then press the “Publish” button to send the price data to the Price Client (IHD).

3.1.9 Messaging Cluster

The “Messaging Cluster” tab can be used to construct and send messages to an IHD or Messaging Client.

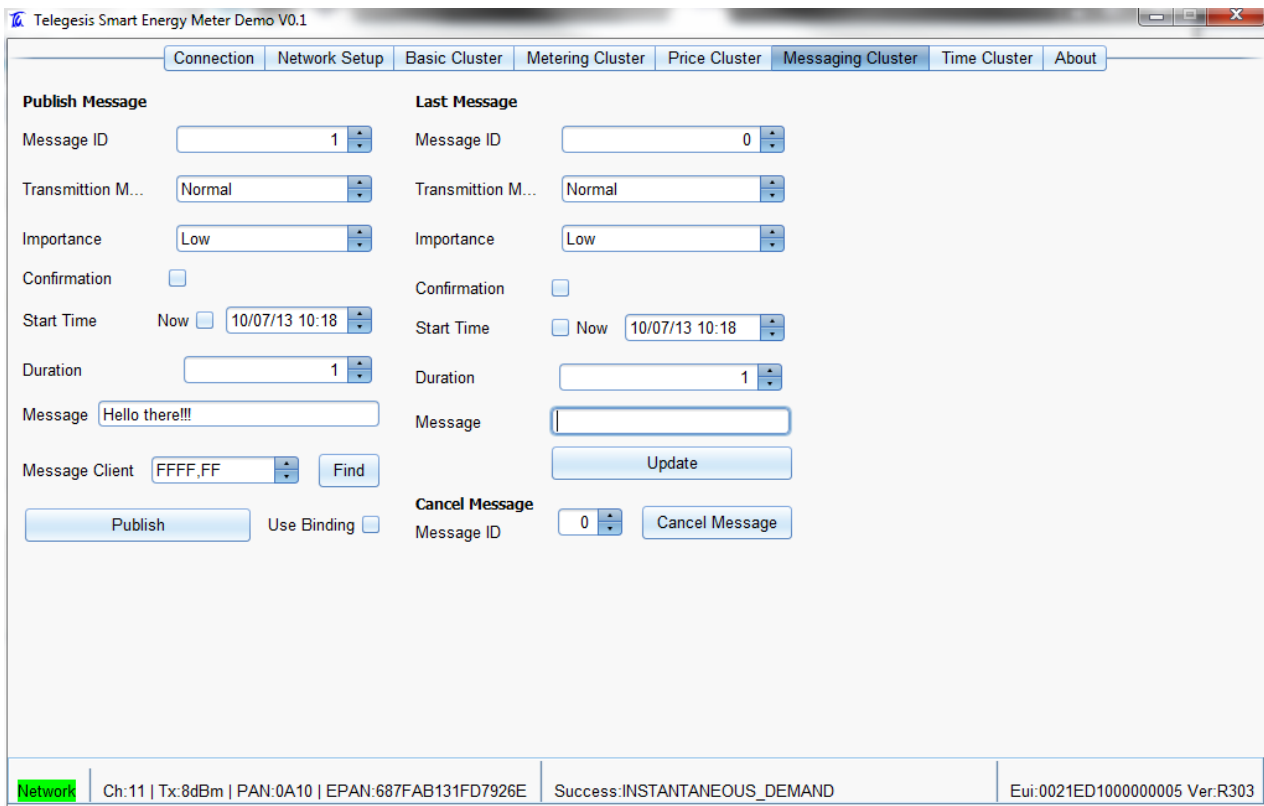

Telegesis Smart Energy Meter Demo V0.1

Connection Network Setup Basic Cluster Metering Cluster Price Cluster **Messaging Cluster** Time Cluster About

Publish Message

Message ID: 1

Transmission M...: Normal

Importance: Low

Confirmation: ☐

Start Time: Now ☐ 10/07/13 10:18

Duration: 1

Message: Hello there!!!

Message Client: FFFF,FF

Use Binding ☐

Last Message

Message ID: 0

Transmission M...: Normal

Importance: Low

Confirmation: ☐

Start Time: ☐ Now 10/07/13 10:18

Duration: 1

Message:

Cancel Message

Message ID: 0

Network | Ch: 11 | Tx: 8dBm | PAN: 0A10 | EPAN: 687FAB131FD7926E | Success: INSTANTANEOUS_DEMAND | Eui: 0021ED1000000005 Ver: R303

Fill in the required fields appropriately in compliance with the ZSE1.1 specification and publish the message using either “Use Binding” to send to all Messaging Clients listed in the binding table or to an individual Message Client by either discovering it using “Find” or by supplying its node ID and endpoint and then clicking the “Publish” button.

The published messages can be cancelled using “Cancel Message” button; the message ID must match the message to be cancelled.

Once a message is published it is copied to the “Last Message” storage of the Mock Meter ETRX3USB and can be retrieved by a Messaging Client if that Message Client missed the message when sent by the Mock Meter.

3.2 In-Premise Display (IHD)


3.2.1 Connection

Insert the Mock Meter ETRX3USB into a USB slot on the PC

If necessary, use the Windows Device Manager to find the COM port number of the Mock Meter.


Start the SEMeter application from the Windows Start Menu

The following screen will be shown:

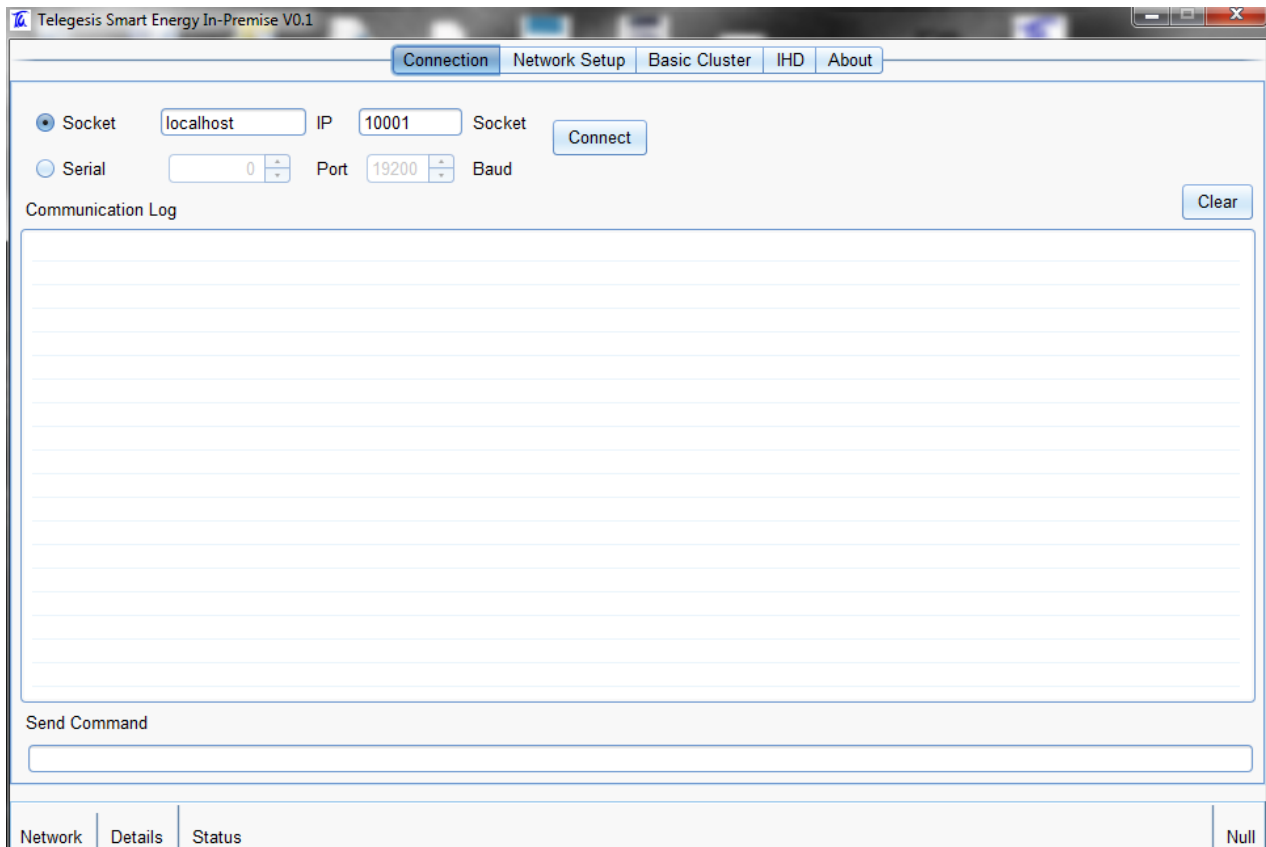

Click on the “Serial” radio button and select the serial port from the adjacent field. Click “Connect” to attempt to connect.

If the connection is successful the status bar is updated with the Mock Meter information and the ZigBee setup stored in the IPD ETRX3USB is retrieved as shown in the screenshot below,

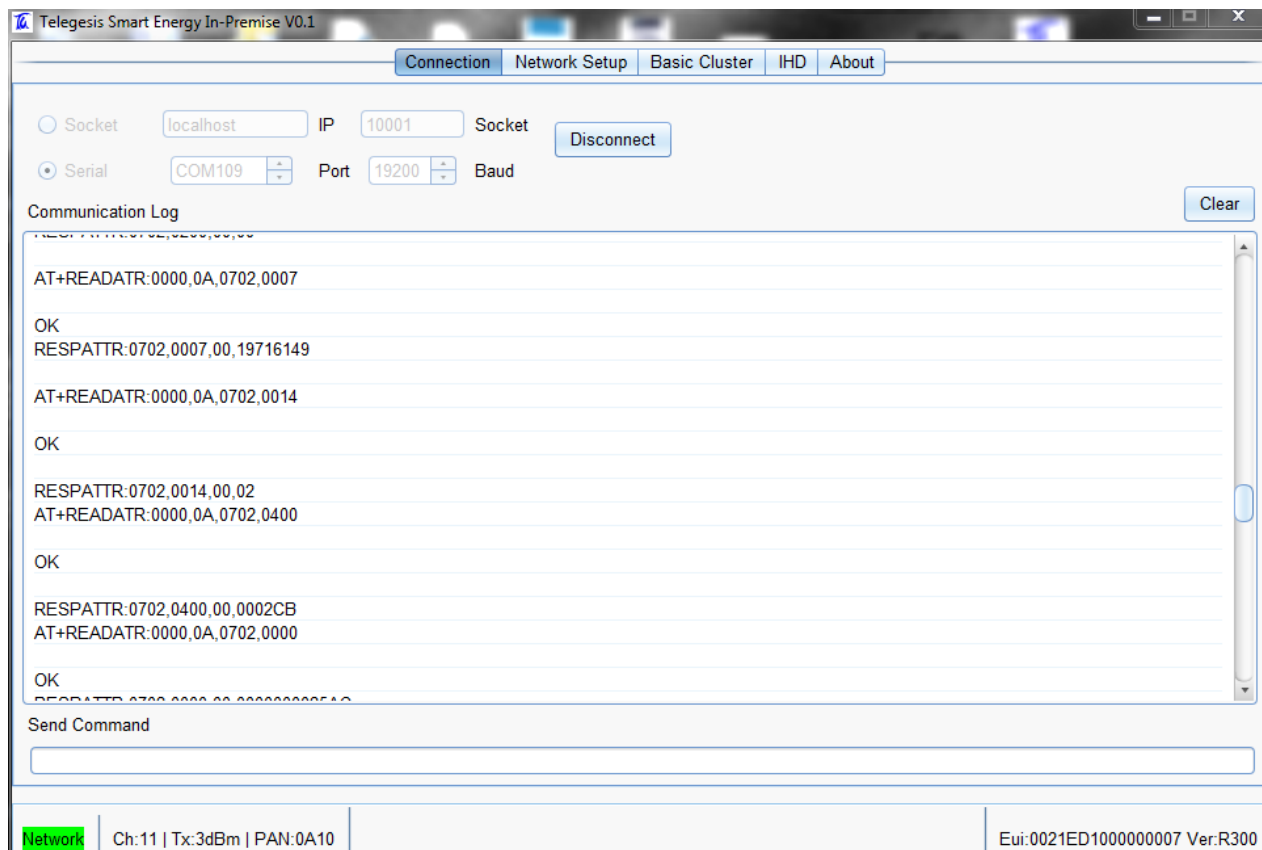


If the selected Serial Port does not connect to an IPD ETRX3USB then an error is shown in the status bar.

All the messages exchanged between an IPD ETRX3USB and the demonstration application are listed in the “Communication Log” window for reference and debugging. AT Commands can also be sent to the IPD ETRX3USB by typing them into the “Send Command” field and pressing the “Enter” key.

3.2.2 Network Joining

Navigate to the “Network Setup” tab and observe the following screen:

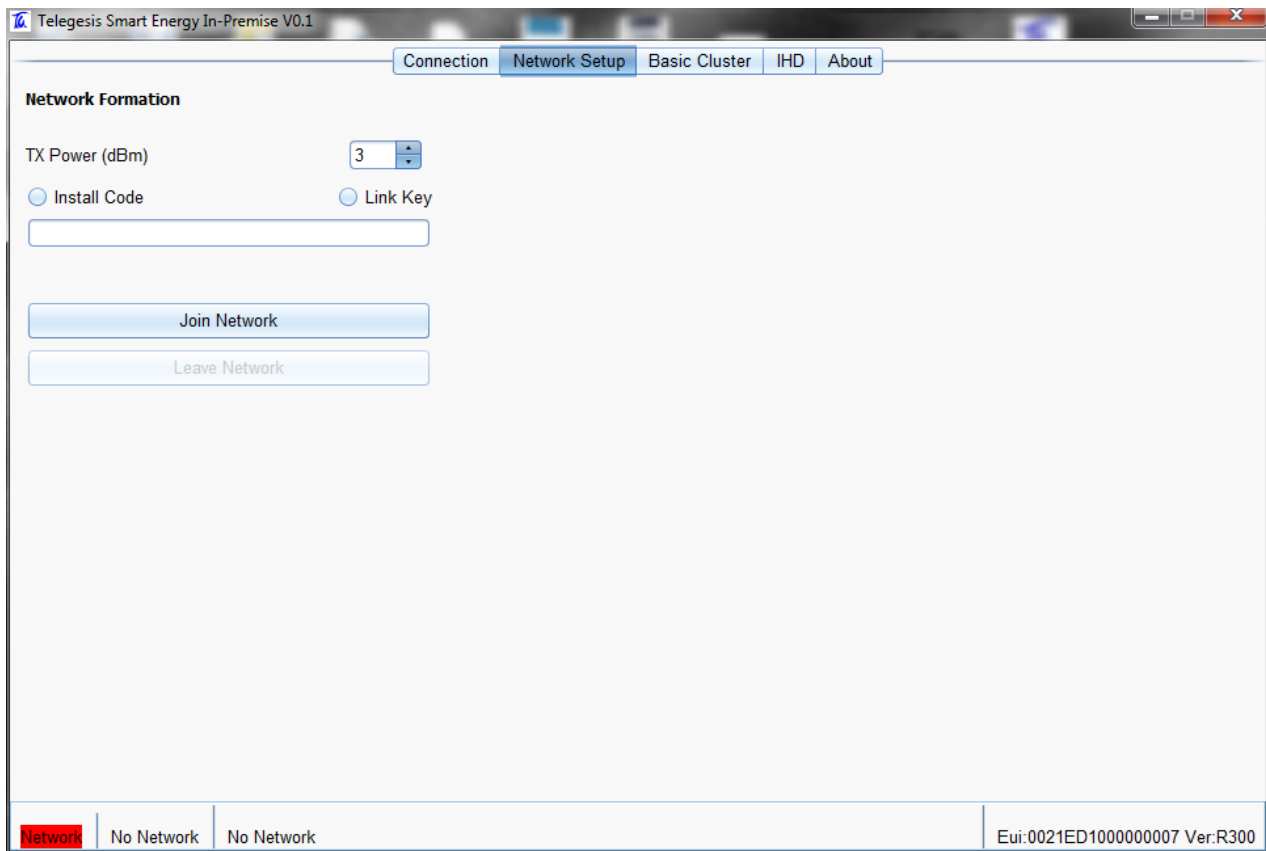

The screenshot shows the "Telegesis Smart Energy In-Premise V0.1" application window. The "Network Setup" tab is selected, showing a "Network Formation" section. It includes a "TX Power (dBm)" spinner set to 3, and two radio buttons: "Install Code" and "Link Key". Below the radio buttons is a text input field. At the bottom of the main area are two buttons: "Join Network" and "Leave Network". The status bar at the bottom shows three indicators: "Network" (highlighted in red), "No Network", and "No Network". On the right side of the status bar, it displays "Eui:0021ED1000000007 Ver:R300".


Select the radio transmit power by changing the “TX Power (dBm)” as shown above. Select “Link Key” or “Install Code” and type an appropriate value in the given field. If “Install Code” is selected the value field is automatically updated with the current value of the Install Code. The Install Code or Link Key must match to the data entered in the “Link Key Table” regarding the In-Premise Display. Press “Join Network” to attempt to join a smart energy network. Success or error will be shown in the status bar as per the outcome of the joining attempt.

The In-Premise Display upon joining the Mock Meter ETRX3USB will go through Smart Energy Registration process which may take a little time; the progress of the Registration process can be monitored in the “Communication Log” window and by the status bar messages.

To leave the ZigBee network press “Leave Network”. The status bar will change to reflect the network state of the device.

3.2.3 Basic Cluster

The Basic Cluster is mandatory for all devices in ZigBee Smart Energy Network. The attributes of the Basic Cluster hosted by the In-Premise Display ETRX3USB can be seen by navigating to the “Basic Cluster” tab in the application. The following screen illustrates the Basic Cluster default settings in the In-Premise Display ETRX3USB:

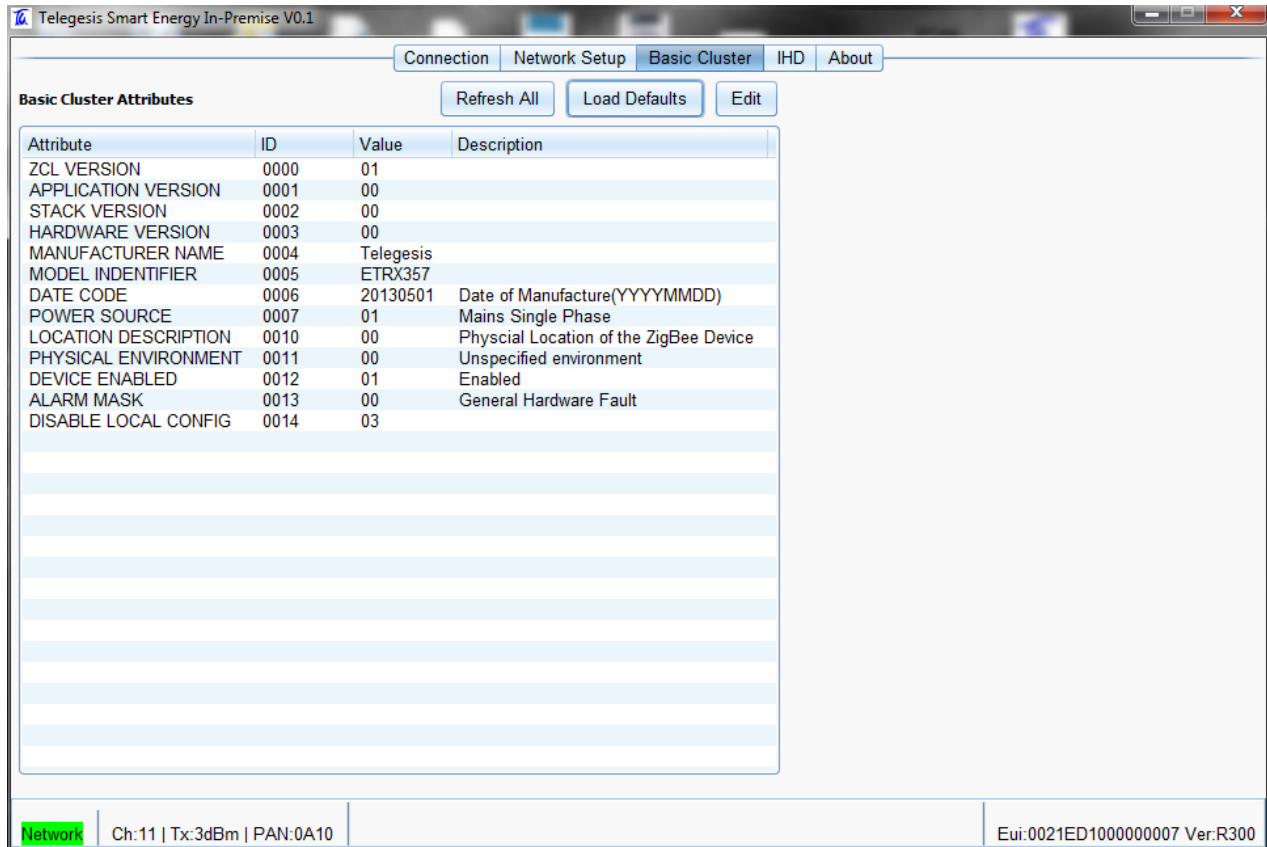

The screenshot shows the 'Basic Cluster Attributes' window of the Telegesis Smart Energy In-Premise V0.1 application. The window has tabs for 'Connection', 'Network Setup', 'Basic Cluster' (selected), 'IHD', and 'About'. Below the tabs are buttons for 'Refresh All', 'Load Defaults', and 'Edit'. The main area contains a table with the following data:

Attribute	ID	Value	Description
ZCL VERSION	0000	01	
APPLICATION VERSION	0001	00	
STACK VERSION	0002	00	
HARDWARE VERSION	0003	00	
MANUFACTURER NAME	0004	Telegesis	
MODEL IDENTIFIER	0005	ETRX357	
DATE CODE	0006	20130501	Date of Manufacture(YYYYMMDD)
POWER SOURCE	0007	01	Mains Single Phase
LOCATION DESCRIPTION	0010	00	Physical Location of the ZigBee Device
PHYSICAL ENVIRONMENT	0011	00	Unspecified environment
DEVICE ENABLED	0012	01	Enabled
ALARM MASK	0013	00	General Hardware Fault
DISABLE LOCAL CONFIG	0014	03	


At the bottom of the window, there is a status bar with the following information: **Network** | Ch:11 | Tx:3dBm | PAN:0A10 | Eui:0021ED1000000007 Ver:R300

All the attributes listed in the table above can be changed by double clicking on the attribute row or by clicking on the “Edit” button.

Please ensure that when updating the attributes the data must conform to the specifications to ensure proper application behaviour.


3.2.4 IHD

The IHD tab shows a representation of a basic In-Premise Display. All fields in this view are automatically updated. By default the In-Premise Display retrieves the attributes from the Mock Meter ETRX3USB every 5 seconds.

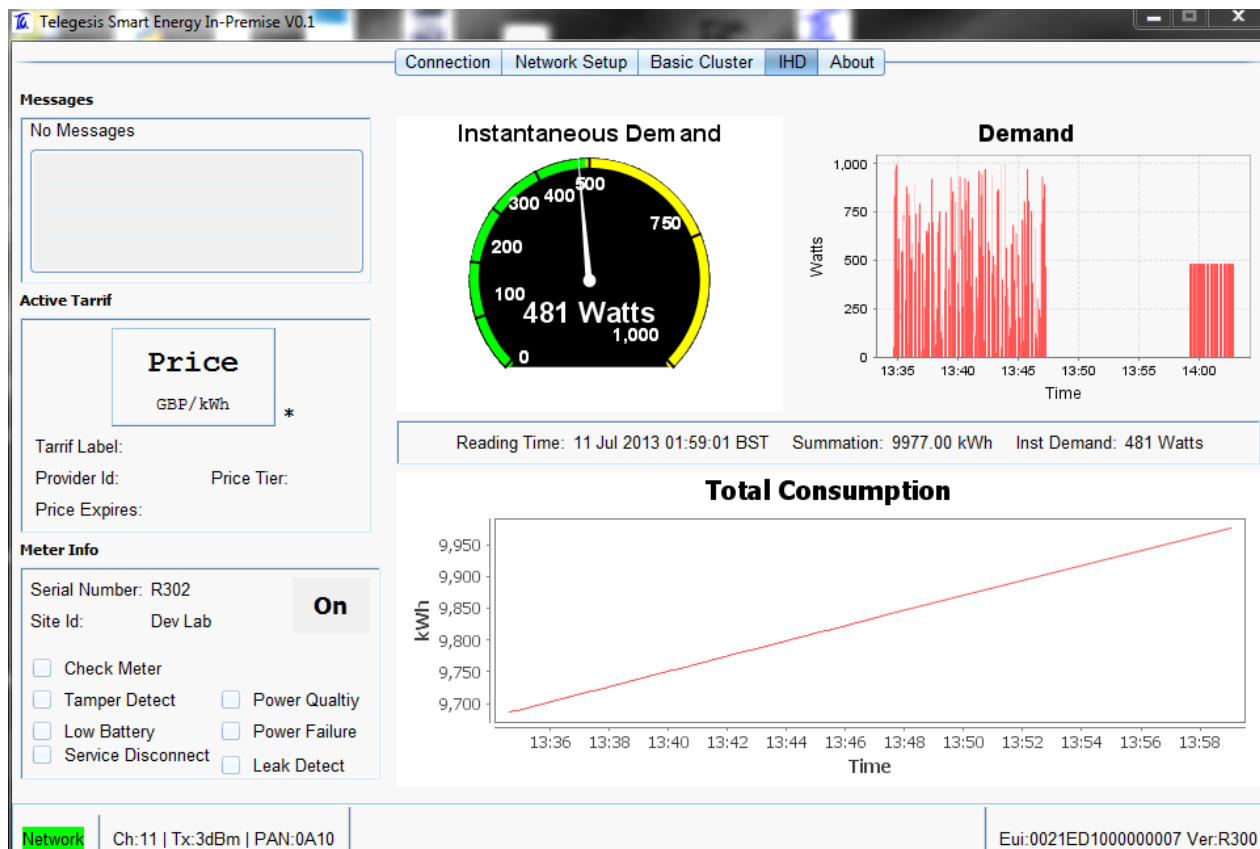

A brief description of the view shown above is as follows.


3.2.4.1 Instantaneous Demand

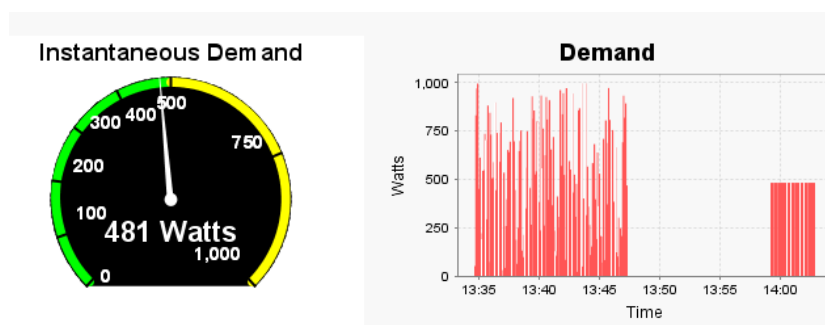

This part shows the Instantaneous Demand attribute as received from Mock Meter ETRX3USB as a meter dial as well as plotted in a chart against time. This visualization is updated periodically at an interval of 5 seconds.


3.2.4.2 Total Summation

The Total Summation attribute is retrieved from the Mock Meter ETRX3USB every 5 seconds and is then plotted against time on the chart shown below,

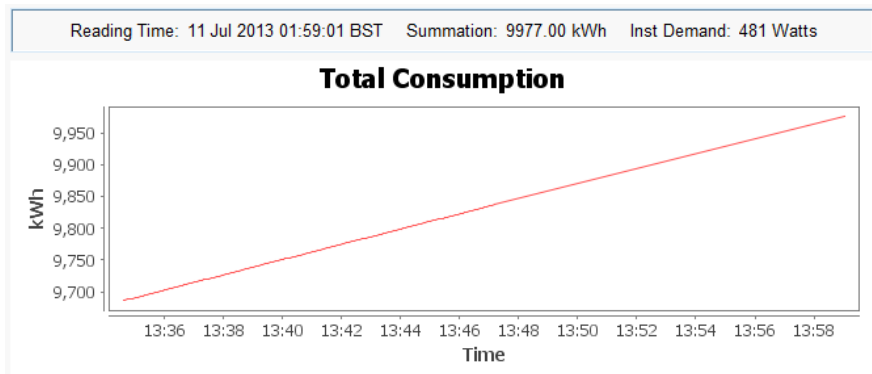


3.2.4.3 Meter Information and Status

The screenshot below shows the Meter information and its status.

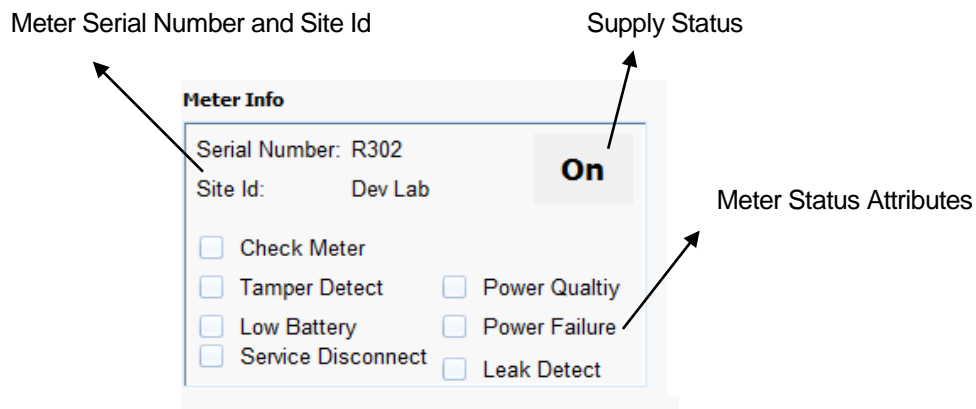

3.2.4.4 Messages


The messages received from the Mock Meter ETRX3USB are displayed in the section shown below with Message Id and duration. Once the duration has elapsed or a Cancel Message command is received the message will be removed from the view.

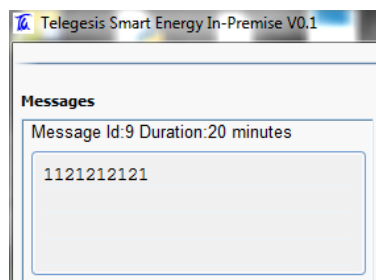

3.2.4.5 Price

Price information as received from the Mock Meter ETRX3USB is shown as below,


Active Tarrif	
0.0900	
GBP / kWh	
Tarrif Label: Normal	
Provider Id: 00000001 Price Tier: 1	
Price Expires: 11 Jul 2013 03:11:36 BST	

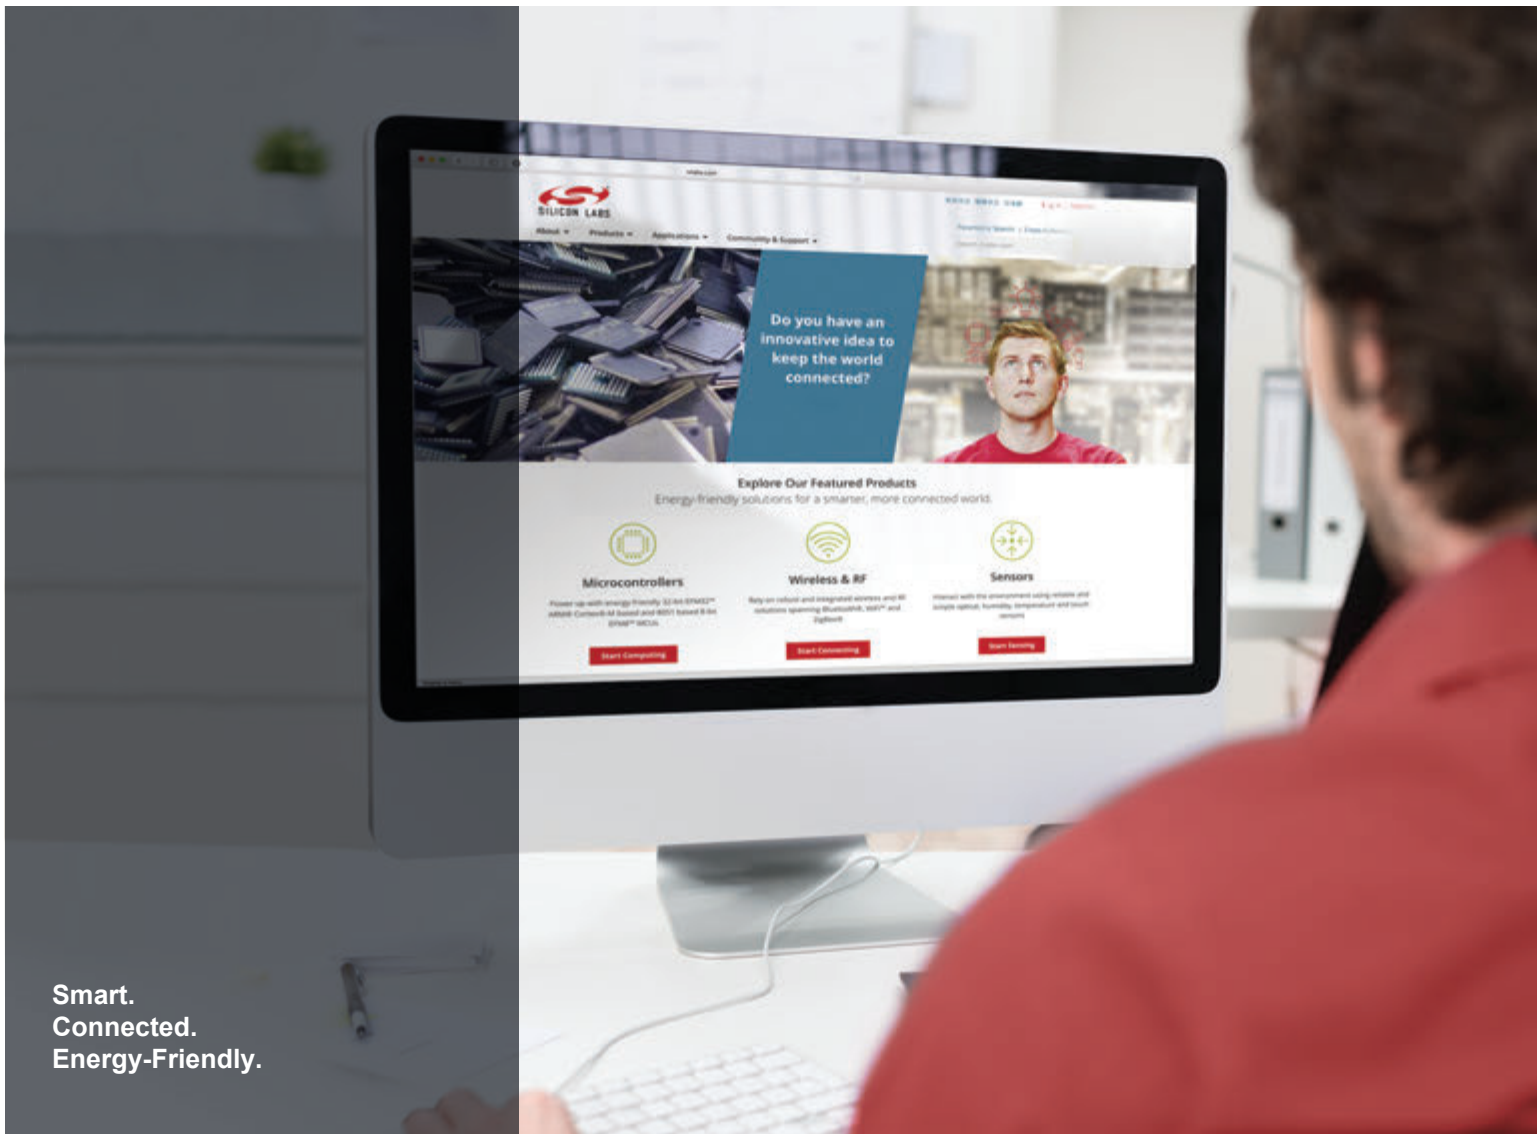

Smart.
Connected.
Energy-Friendly.



Products
www.silabs.com/products



Quality
www.silabs.com/quality



Support and Community
community.silabs.com

Disclaimer

Silicon Laboratories intends to provide customers with the latest, accurate, and in-depth documentation of all peripherals and modules available for system and software implementers using or intending to use the Silicon Laboratories products. Characterization data, available modules and peripherals, memory sizes and memory addresses refer to each specific device, and "Typical" parameters provided can and do vary in different applications. Application examples described herein are for illustrative purposes only. Silicon Laboratories reserves the right to make changes without further notice and limitation to product information, specifications, and descriptions herein, and does not give warranties as to the accuracy or completeness of the included information. Silicon Laboratories shall have no liability for the consequences of use of the information supplied herein. This document does not imply or express copyright licenses granted hereunder to design or fabricate any integrated circuits. The products are not designed or authorized to be used within any Life Support System without the specific written consent of Silicon Laboratories. A "Life Support System" is any product or system intended to support or sustain life and/or health, which, if it fails, can be reasonably expected to result in significant personal injury or death. Silicon Laboratories products are not designed or authorized for military applications. Silicon Laboratories products shall under no circumstances be used in weapons of mass destruction including (but not limited to) nuclear, biological or chemical weapons, or missiles capable of delivering such weapons.

Trademark Information

Silicon Laboratories Inc.®, Silicon Laboratories®, Silicon Labs®, SiLabs® and the Silicon Labs logo®, Bluegiga®, Bluegiga Logo®, Clockbuilder®, CMEMS®, DSPLL®, EFM®, EFM32®, EFR®, Ember®, Energy Micro, Energy Micro logo and combinations thereof, "the world's most energy friendly microcontrollers", Ember®, EZLink®, EZRadio®, EZRadioPRO®, Gecko®, ISOmodem®, Precision32®, ProSLIC®, Simplicity Studio®, SiPHY®, Telegesis, the Telegesis Logo®, USBXpress® and others are trademarks or registered trademarks of Silicon Laboratories Inc. ARM, CORTEX, Cortex-M3 and THUMB are trademarks or registered trademarks of ARM Holdings. Keil is a registered trademark of ARM Limited. All other products or brand names mentioned herein are trademarks of their respective holders.



Silicon Laboratories Inc.
400 West Cesar Chavez
Austin, TX 78701
USA

<http://www.silabs.com>